

Test report

Customer:

SOEKS Limited Liability Company

Altuflevskoye shosse,h.48,bld.1pr.1,room39
Moscow,127566
Russia

EMC test report 130504-AU01+E02



SOEKS Limited Liability Company

Nitrate testing device

NUC-019-1



This test report may not be copied
or published in a part without
the written authorization
of the accreditation agency and/or
EMV **TESTHAUS** GmbH
Revision: 1.3



EMV **TESTHAUS** GmbH

Gustav-Hertz-Straße 35
94315 Straubing Tel.:
+49 9421 56868-0
Fax: +49 9421 56868-100

Accreditation:



Location of Testing:

EMV **TESTHAUS** GmbH
Gustav-Hertz-Straße 35
94315 Straubing

The technical accuracy is guaranteed through the quality management of the
EMV **TESTHAUS** GmbH.



EMV **TESTHAUS** GmbH
Gustav-Hertz-Straße 35
94315 Straubing
Germany
Revision: 1.3

SOEKS Limited Liability Company
Nitrate testing device
NUC-019-1

130504-AU01+E02

Page 2 of 24

Table of contents

| | |
|---|----|
| 1. Test regulation | 4 |
| 2. Equipment under test | 8 |
| 3. Test configuration and mode of operation | 10 |
| 4. Measurement of radiated emission | 11 |
| 5. Electrostatic discharge immunity test | 15 |
| 6. Radiated, radio-frequency, electromagnetic field immunity test | 19 |
| 7. Measurement uncertainty | 23 |
| 8. Summary | 24 |



EMV **TESTHAUS** GmbH
Gustav-Hertz-Straße 35
94315 Straubing
Germany
Revision: 1.3

SOEKS Limited Liability Company
Nitrate testing device
NUC-019-1

130504-AU01+E02

Page 3 of 24

1. Test regulation

Emission

EN 55011:2009
+A1:2010

Industrial, scientific and medical (ISM)
radio-frequency - Radio disturbance
characteristics -
Limits and methods of measurement

☒ Group 1

Group 1 contains all ISM equipment in which there is intentionally generated and/or used conductively coupled radio-frequency energy which is necessary for the internal functioning of the equipment itself.

☐ Group 2

Group 2 contains all ISM equipment in which radio-frequency energy is intentionally generated and/or used in the form of electromagnetic radiation for the treatment of material, and spark erosion equipment.

☐ Class A

Class A equipment is equipment suitable for use in all establishments other than domestic and those directly connected to a low voltage power supply network which supplies buildings used for domestic purposes.

☒ Class B:

Class B equipment is equipment suitable for use in domestic establishments and in establishments directly connected to a low voltage power supply network which supplies buildings used for domestic purposes.



EMV **TESTHAUS** GmbH
Gustav-Hertz-Straße 35
94315 Straubing
Germany
Revision: 1.3

SOEKS Limited Liability Company
Nitrate testing device
NUC-019-1

130504-AU01+E02

Page 4 of 24

Includes the following tests:

EN 55011:2009 +A1:2010 Measurement of the conducted disturbance at mains ports in a frequency range from 150 kHz to 30 MHz.

Measurement of radiated disturbance in a frequency range from 30 MHz to 1 GHz.

Emission in the frequency range of ≤ 2 kHz:

EN 61000-3-2:2006 Harmonic current emissions
(equipment input current ≤ 16 A per phase)

EN 61000-3-3:1995
+ A1:2001 Limitation of voltage fluctuations and flicker in low-voltage supply systems for equipment with rated current ≤ 16 A

Deviation of regulations and standards: No



EMV **TESTHAUS** GmbH
Gustav-Hertz-Straße 35
94315 Straubing
Germany
Revision: 1.3

SOEKS Limited Liability Company
Nitrate testing device
NUC-019-1

130504-AU01+E02

Page 5 of 24

Susceptibility

EN 61326-1:2006

Electrical equipment for measurement, control and laboratory use- EMC requirements - Part 1: General requirements.

Includes Basic EMC Publications:

EN 61000-4-2:1995
+ A1:1998 + A2:2001

Testing and measurement techniques - Electrostatic discharge immunity test.

EN 61000-4-3:2002

Testing and measurement techniques - Radiated, radio frequency, immunity test.

EN 61000-4-4:2004

Testing and measurement techniques - Electrical fast transient (EFT)/burst immunity test.

EN 61000-4-5:1995
+ A1:2001

Testing and measurement techniques - Surge immunity test.

EN 61000-4-6:1996
+ A1:2001

Testing and measurement techniques - Immunity to conducted disturbances, induced by radio-frequency fields.

EN 61000-4-8:1993
+ A1:2001

Testing and measurement techniques - Power frequency magnetic field immunity test.

EN 61000-4-11:2004

Testing and measurement techniques - Voltage dips, short interruptions and voltage variations immunity tests.

Deviation of Regulation and Standards: No



EMV **TESTHAUS** GmbH
Gustav-Hertz-Straße 35
94315 Straubing
Germany
Revision: 1.3

SOEKS Limited Liability Company
Nitrate testing device
NUC-019-1

130504-AU01+E02

Page 6 of 24

Not applied tests:

| | |
|--------------------------------|---|
| EN 55011:2009 +A1:2010 | Measurement of the conducted disturbance at mains ports in a frequency range from 150 kHz to 30 MHz. |
| EN 61000-3-2:2006 | Harmonic current emissions (equipment input current ≤ 16 A per phase) |
| EN 61000-3-3:1995 + A1:2001 | Limitation of voltage fluctuations and flicker in low-voltage supply systems for equipment with rated current ≤ 16 A |
| EN 61000-4-4:2004 | Testing and measurement techniques - Electrical fast transient (EFT)/burst immunity test. |
| EN 61000-4-5:1995 + A1:2001 | Testing and measurement techniques - Surge immunity test. |
| EN 61000-4-6:1996 + A1:2001 | Testing and measurement techniques - Immunity to conducted disturbances, induced by radio-frequency fields. |
| EN 61000-4-11:2004 | Testing and measurement techniques - Voltage dips, short interruptions and voltage variations immunity tests. |
| Remark: | The EUT is battery powered. |
| EN 61000-4-8:1993 + A1:2001 | Testing and measurement techniques - Power frequency magnetic field immunity test. |
| Remark: | Only for equipment containing devices susceptible to magnetic fields. |



2. Equipment under test

Product type: Nitrate testing device
Model name: NUC-019-1
Serial number: N/A
Manufacturer: SOEKS Limited Liability Company

www.dozimetr.biz



EMV **TESTHAUS** GmbH
Gustav-Hertz-Straße 35
94315 Straubing
Germany
Revision: 1.3

SOEKS Limited Liability Company
Nitrate testing device
NUC-019-1

130504-AU01+E02

Page 8 of 24

Photo documentation



Picture 1: Equipment under test

3. Test configuration and mode of operation

Test configuration

| Device | Model: | S/N |
|------------------------|-----------|-----|
| Nitrate testing device | NUC-019-1 | N/A |

Mode of operation

The EUT was tested in the following mode of operation:

Settings: measuring

Applied Software: None

Failure criterion for test of immunity from disturbances:

It was observed whether the EUT is influenced in any form or program interruptions occurred.



EMV **TESTHAUS** GmbH
Gustav-Hertz-Straße 35
94315 Straubing
Germany
Revision: 1.3

SOEKS Limited Liability Company
Nitrate testing device
NUC-019-1

130504-AU01+E02

Page 10 of 24

4. Measurement of radiated emission

according to EN 55011 Group 1 Class B

Procedure of radiated emission measurement:

- ☒ Scan with max-peak detector in 3 m CDC
- ☒ Final CISPR measurement with quasi peak detector on 10m open area test site

Location of measurement

| Description | Manufacturer | Inventory No. |
|---------------------|--------------------------|---------------|
| CDC | Albatross Projects | E00026 |
| Open area test site | EMV TESTHAUS GmbH | E00354 |

Measurement equipment

| | Description | Manufacturer | Inventory No. |
|-------------------------------------|------------------|-----------------|---------------|
| <input checked="" type="checkbox"/> | ESCI (CDC) | Rohde & Schwarz | E00001 |
| <input type="checkbox"/> | ESU26 | Rohde & Schwarz | W00002 |
| <input checked="" type="checkbox"/> | ESCS 30 (OATS) | Rohde & Schwarz | E00003 |
| <input checked="" type="checkbox"/> | VULB 9160 (CDC) | Schwarzbeck | E00011 |
| <input checked="" type="checkbox"/> | VULB 9163 (OATS) | Schwarzbeck | E00012 |

Test related measurement inaccuracies have to be taken into consideration when evaluating the test results.
All used test instrument as well as the test accessories are calibrated at regular intervals.




EMV **TESTHAUS** GmbH
Gustav-Hertz-Straße 35
94315 Straubing
Germany
Revision: 1.3

SOEKS Limited Liability Company
Nitrate testing device
NUC-019-1

130504-AU01+E02

Page 11 of 24

Interference Radiation Test

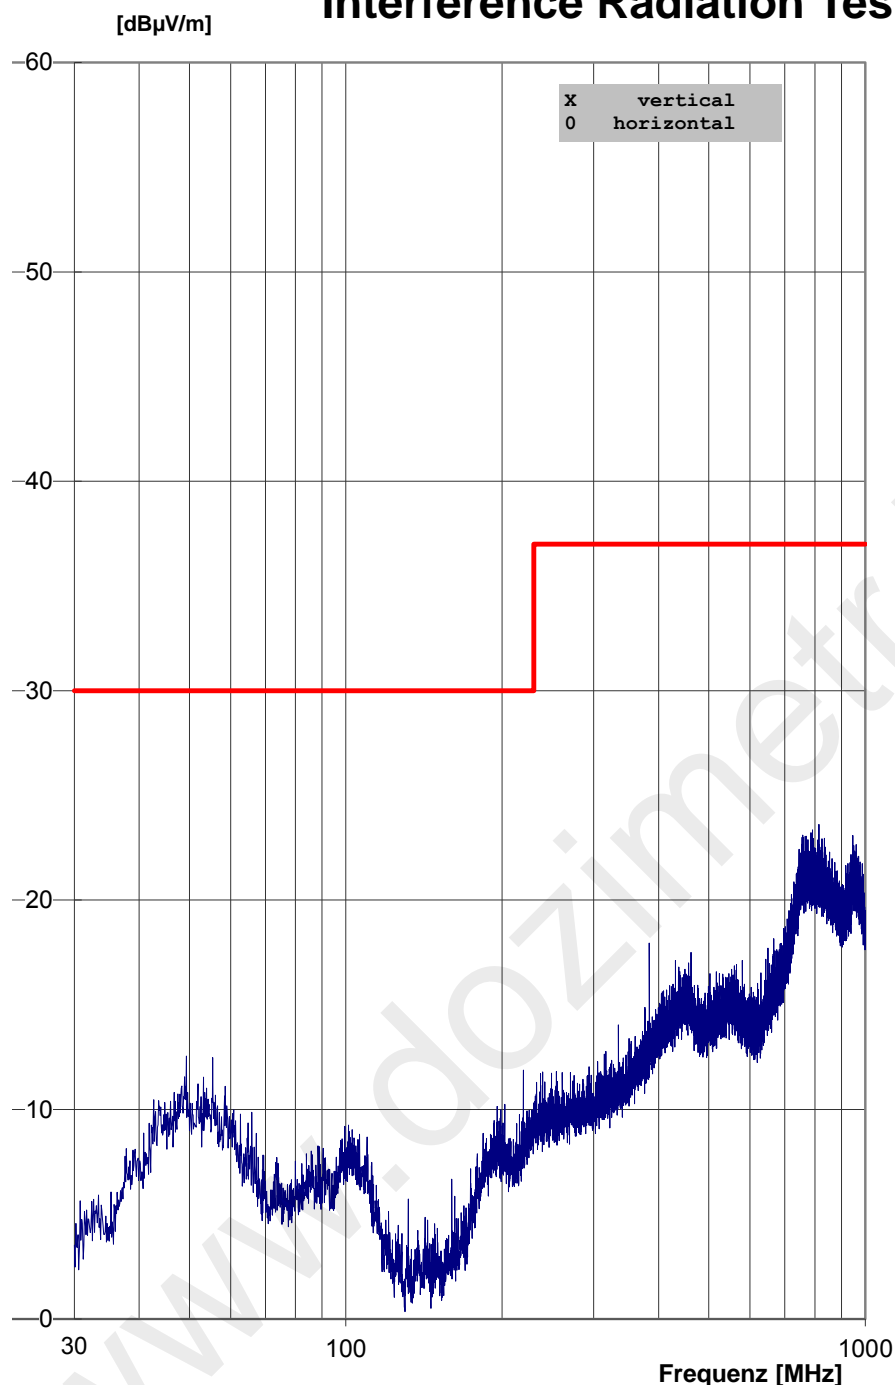

REGULATIONS:
EN 55011 Group 1 Class B
PEAK / CISPR

TEST EQUIPMENT:
R&S ESCS30 (E00003)
VULB 9163 (E00013)

ORDER NO.:
130504-AU01+E02

EUT:
SOEKS Limited Liability
Company
Nitrate testing device
NUC-019-1

OPERATION MODE:
measuring

TEST FACILITY:
EMV TESTHAUS GmbH
Gustav-Hertz-Straße 35
94315 Straubing

DATE / TIME:
2014-01-20 10:28:14
2,7°C, 100%, 101kPa

TEST ENGINEER:
Martin Müller

130504-AU01+E02 OATS.E10

Picture 2: Measurement report of radiated emission




EMV **TESTHAUS** GmbH
Gustav-Hertz-Straße 35
94315 Straubing
Germany
Revision: 1.3

SOEKS Limited Liability Company
Nitrate testing device
NUC-019-1

130504-AU01+E02

Page 12 of 24

Photo documentation

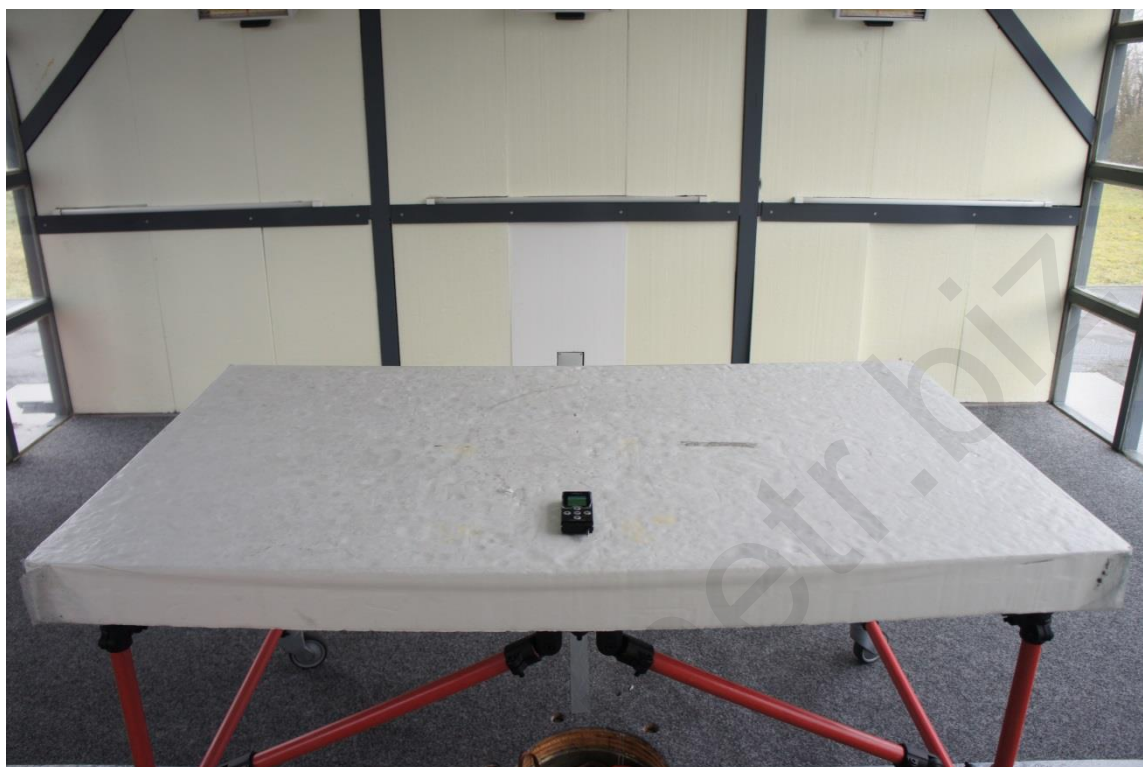

Picture 3: Test setup radiated emission

Test result

The requirements according to EN 55011 Group 1 Class B are

☒ **Kept**

☐ **Not kept**

Information about measurement uncertainty is on page 23.

www.dozimetr.biz



EMV **TESTHAUS** GmbH
Gustav-Hertz-Straße 35
94315 Straubing
Germany
Revision: 1.3

SOEKS Limited Liability Company
Nitrate testing device
NUC-019-1

130504-AU01+E02

Page 14 of 24

5. Electrostatic discharge immunity test

according to EN 61000-4-2

Location of measurement

| Description | Manufacturer | Inventory No. |
|------------------|----------------------|---------------|
| Shielded chamber | Siemens - Matsushita | E00107 |

Measurement equipment

| | Description | Manufacturer | Inventory No. |
|-------------------------------------|-------------|--------------------------|---------------|
| <input type="checkbox"/> | ESD 3000 | EMC Partner | E00040 |
| <input checked="" type="checkbox"/> | NSG 435 | Teseq | E00412 |
| <input checked="" type="checkbox"/> | VCP | EMV TESTHAUS GmbH | E00047 |
| <input checked="" type="checkbox"/> | HCP | EMV TESTHAUS GmbH | E00048 |

Test related measurement inaccuracies have to be taken into consideration when evaluating the test results.
All used test instrument as well as the test accessories are calibrated at regular intervals.



EMV **TESTHAUS** GmbH
Gustav-Hertz-Straße 35
94315 Straubing
Germany
Revision: 1.3

SOEKS Limited Liability Company
Nitrate testing device
NUC-019-1

130504-AU01+E02

Page 15 of 24

Test conditions

Air discharge

Test voltage:

| | | |
|-------------------------------------|-------|--------------|
| <input checked="" type="checkbox"/> | 2 kV | test level 1 |
| <input checked="" type="checkbox"/> | 4 kV | test level 2 |
| <input checked="" type="checkbox"/> | 8 kV | test level 3 |
| <input type="checkbox"/> | 15 kV | test level 4 |
| <input type="checkbox"/> | kV | test level x |

Polarity:

| | |
|-------------------------------------|----------|
| <input checked="" type="checkbox"/> | positive |
| <input checked="" type="checkbox"/> | negative |

Discharges: ≥ 10 discharges per polarity

Discharging points: screws, housing slots
no discharges

Contact discharge

Test voltage:

| | | |
|-------------------------------------|------|--------------|
| <input checked="" type="checkbox"/> | 2 kV | test level 1 |
| <input checked="" type="checkbox"/> | 4 kV | test level 2 |
| <input type="checkbox"/> | 6 kV | test level 3 |
| <input type="checkbox"/> | 8 kV | test level 4 |
| <input type="checkbox"/> | kV | test level x |

Polarity:

| | |
|-------------------------------------|----------|
| <input checked="" type="checkbox"/> | positive |
| <input checked="" type="checkbox"/> | negative |

Discharges: ≥ 10 discharges per polarity

Discharging points:

| | |
|---------|---|
| direct: | USB shield, measuring probe no discharges |
|---------|---|

indirect: HCP, VCP

Climatic conditions:

| | |
|----------------------|---------|
| Ambient temp.: | 21,9 °C |
| Relative humidity.: | 32,2 % |
| Barometric pressure: | 97 kPa |




EMV **TESTHAUS** GmbH
Gustav-Hertz-Straße 35
94315 Straubing
Germany
Revision: 1.3

SOEKS Limited Liability Company
Nitrate testing device
NUC-019-1

130504-AU01+E02

Page 16 of 24

Photo documentation

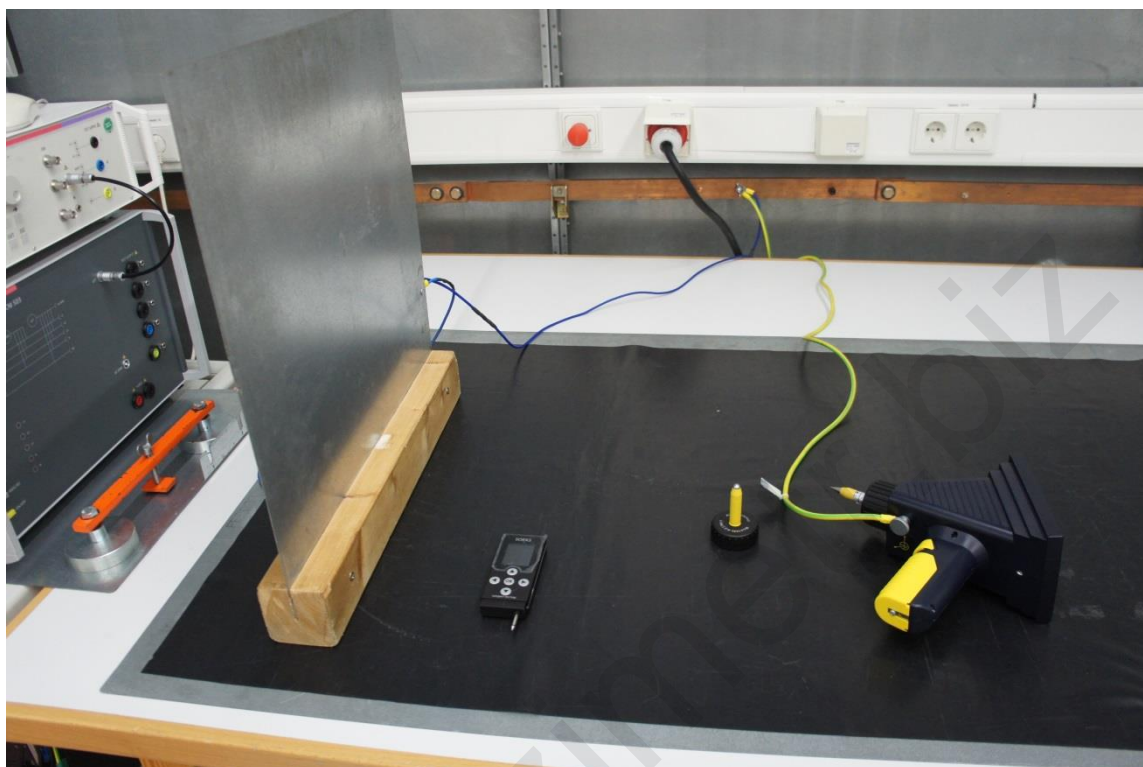

Picture 4: Test setup ESD

Test result

The requirements according to EN 61000-4-2 are

- ☒ **Kept**
- ☐ **Not kept**

Information about measurement uncertainty is on page 23.

Operating conditions during test:

Criterion

- ☒ **A** The equipment shall continue to operate as intended without operator intervention. No degradation of performance or loss of function is allowed below performance level specified by the manufacturer when the equipment is used as intended. The performance level may be replaced by a permissible loss of performance. If the minimum performance level or the permissible performance loss is not specified by the manufacturer, then either of these may be derived from the product description and documentation, and by what the user may reasonably expect from the equipment if used as intended.
- ☐ **B** After the test, the equipment shall continue to operate as intended without operator invention. No degradation of performance or loss of function is allowed, after the application of the phenomena below a performance level specified by the manufacturer, when the equipment is used as intended. The performance level may be replaced by a permissible loss of performance. During the test, degradation of performance is allowed. However, no change of operating state or stored data is allowed to persist after the test. If the minimum performance level (or the permissible performance loss) is not specified by the manufacturer, then either of these may be derived from the product description and documentation, and by what the user may reasonably expect from the equipment if used as intended.
- ☐ **C** Loss of function is allowed, provided the function is self-recoverable, or can be restored by the operation of the controls by the user in accordance with the manufacturer's instructions. Functions, and/or information stored in non-volatile memory, or protected by a battery backup, shall not be lost.

Comments: During the test the function of the EUT was observed. Influences in any form or program interruptions did not occur.



EMV **TESTHAUS** GmbH
Gustav-Hertz-Straße 35
94315 Straubing
Germany
Revision: 1.3

SOEKS Limited Liability Company
Nitrate testing device
NUC-019-1

130504-AU01+E02

Page 18 of 24

6. Radiated, radio-frequency, electromagnetic field immunity test

according to EN 61000-4-3

Location of measurement

| Description | Manufacturer | Inventory No. |
|------------------|--------------------------|---------------|
| Anechoic chamber | EMV TESTHAUS GmbH | E00100 |

Measurement equipment

| | Model | Description | Manufacturer | Inventory |
|-------------------------------------|----------------|-------------------------|-----------------|-----------|
| <input checked="" type="checkbox"/> | VULB 9163 | Antenna 30 – 3000 MHz | Schwarzbeck | E00013 |
| <input checked="" type="checkbox"/> | BBHA 9120E | Antenne 1000 – 2700 MHz | Schwarzbeck | E00018 |
| <input checked="" type="checkbox"/> | SMT06 | Signal Generator | Rohde & Schwarz | E00036 |
| <input checked="" type="checkbox"/> | COSF 3312 | Power Switching Unit | Conformitas | E00037 |
| <input checked="" type="checkbox"/> | NRVD | Power Meter | Rohde & Schwarz | E00038 |
| <input checked="" type="checkbox"/> | AS0104-55/30 | Amplifier 1 - 4GHz | Milmega | E00070 |
| <input checked="" type="checkbox"/> | BT A 0122-150W | Amplifier 9 kHz-220 MHz | Bonn | E00071 |
| <input checked="" type="checkbox"/> | BLWA 2010-100W | Amplifier 200-1000 MHz | Bonn | E00072 |
| <input checked="" type="checkbox"/> | NRV-Z51 | Power Measuring Head | Rohde & Schwarz | E00075 |
| <input checked="" type="checkbox"/> | NRV-Z51 | Power Measuring Head | Rohde & Schwarz | E00076 |

Test related measurement inaccuracies have to be taken into consideration when evaluating the test results.
All used test instrument as well as the test accessories are calibrated at regular intervals.



EMV **TESTHAUS** GmbH
Gustav-Hertz-Straße 35
94315 Straubing
Germany
Revision: 1.3

SOEKS Limited Liability Company
Nitrate testing device
NUC-019-1

130504-AU01+E02

Page 19 of 24

Test Conditions

Frequency range: ☒ 80 MHz - 1000 MHz with test level 3
☒ 1400 MHz - 2000 MHz with test level 2
☒ 2000 MHz - 2700 MHz with test level 1

Step size: ☒ 1 % of output frequency
☐ 4 % of output frequency

Field strength: ☒ 1 V/m test level 1
☒ 3 V/m test level 2
☒ 10 V/m test level 3
☐ V/m test level x

Modulation: Kind of Modulation: AM
Modulation factor: 80 %
Modulation frequency: 1 kHz

Dwell time: ☒ 3 seconds
☐ X seconds

Antenna polarization: ☒ vertical
☒ horizontal

Test distance: ☐ 1 m
☒ 3 m

EUT position: ☒ front side
☒ rear side
☒ left side
☒ right side
☐ top
☐ bottom

Observation of EUT: Via video camera

Climatic conditions: Ambient temp.: 21,9 ° C
Relative humidity.: 32,2 %
Barometric pressure: 97 kPa




EMV **TESTHAUS** GmbH
Gustav-Hertz-Straße 35
94315 Straubing
Germany
Revision: 1.3

SOEKS Limited Liability Company
Nitrate testing device
NUC-019-1

130504-AU01+E02

Page 20 of 24

Photo documentation

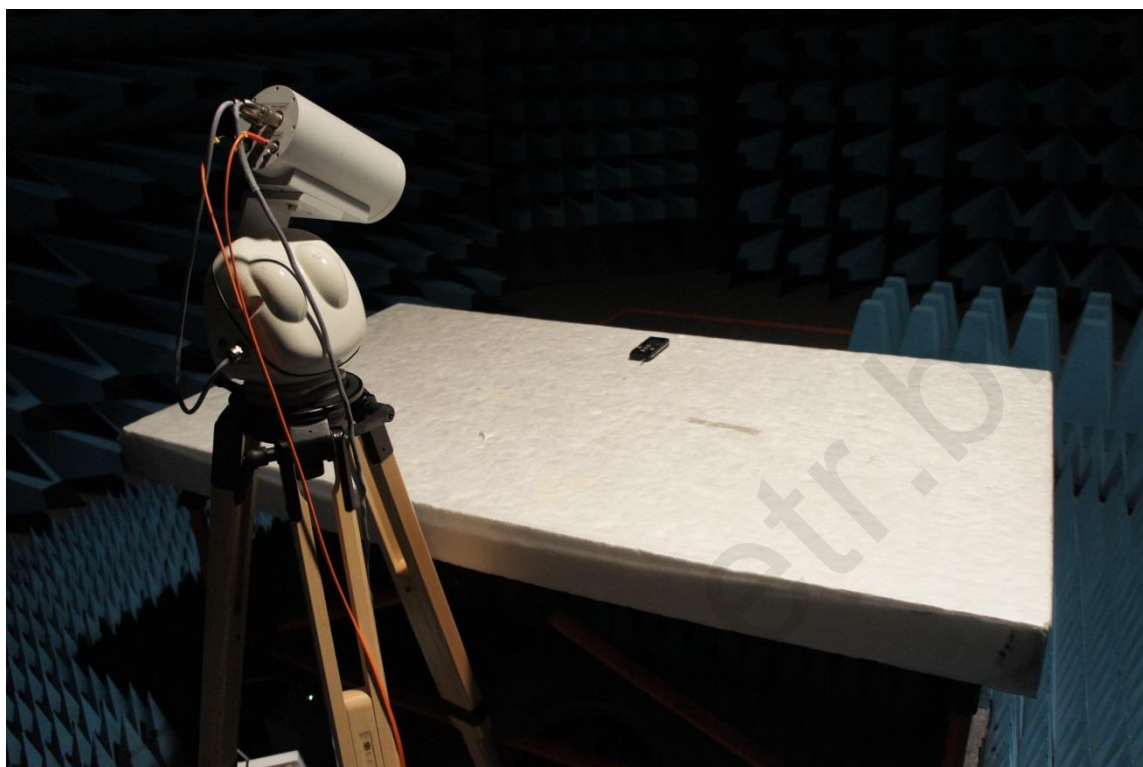

Picture 5: Test setup radiated immunity test

Test result

The requirements according to EN 61000-4-3 are

- ☒ **Kept**
- ☐ **Not kept**

Information about measurement uncertainty is on page 23.

Operating conditions during test:

Criterion

- ☒ **A** The equipment shall continue to operate as intended without operator intervention. No degradation of performance or loss of function is allowed below performance level specified by the manufacturer when the equipment is used as intended. The performance level may be replaced by a permissible loss of performance. If the minimum performance level or the permissible performance loss is not specified by the manufacturer, then either of these may be derived from the product description and documentation, and by what the user may reasonably expect from the equipment if used as intended.
- ☐ **B** After the test, the equipment shall continue to operate as intended without operator intervention. No degradation of performance or loss of function is allowed, after the application of the phenomena below a performance level specified by the manufacturer, when the equipment is used as intended. The performance level may be replaced by a permissible loss of performance. During the test, degradation of performance is allowed. However, no change of operating state or stored data is allowed to persist after the test. If the minimum performance level (or the permissible performance loss) is not specified by the manufacturer, then either of these may be derived from the product description and documentation, and by what the user may reasonably expect from the equipment if used as intended.
- ☐ **C** Loss of function is allowed, provided the function is self-recoverable, or can be restored by the operation of the controls by the user in accordance with the manufacturer's instructions. Functions, and/or information stored in non-volatile memory, or protected by a battery backup, shall not be lost.

Comments: During the test the function of the EUT was observed. Influences in any form or program interruptions did not occur.



EMV **TESTHAUS** GmbH
Gustav-Hertz-Straße 35
94315 Straubing
Germany
Revision: 1.3

SOEKS Limited Liability Company
Nitrate testing device
NUC-019-1

130504-AU01+E02

Page 22 of 24

7. Measurement uncertainty

| Standard | Description | Max. deviation | k= |
|---------------|--|---------------------------|------|
| EN 55011 | Conducted emission AMN (150kHz to 30 MHz) | +/- 4,1 dB | 2 |
| EN 55011 | Radiated emission open field (30 MHz to 300 MHz) (300MHz to 1 GHz) | +/- 5,4 dB +/- 4,7 dB | 2 |
| EN 61000-4-2 | ESD | inside specification * | |
| EN 61000-4-3 | Radiated immunity | +/- 1,8 dB ^{a.)} | 1,64 |
| EN 61000-4-4 | Burst | inside specification * | |
| EN 61000-4-5 | Surge | inside specification * | |
| EN 61000-4-6 | Conducted immunity with CDN (150 kHz to 230 MHz) | +/- 2,4 dB ^{b.)} | 1,64 |
| EN 61000-4-6 | Conducted immunity with BCI (150 kHz to 230 MHz) | +/- 2,4 dB ^{c.)} | 1,64 |
| EN 61000-4-8 | Magnetic field | +/- 0,9 dB | 2 |
| EN 61000-4-11 | Dips | inside specification * | 2 |
| EN 61000-3-2 | Harmonic currents | +/- 0,2 % ^{d.)} | 1 |
| EN 61000-3-3 | Flicker | annotation ^{e.)} | |

Comment: The uncertainty stated is the expanded uncertainty obtained by multiplying the standard uncertainty by the coverage factor k. If k=2 the value of the measurands lies within the assigned range of values with a probability of 95 %.

- * The specific requirements regarding to the standard was kept
- a.) To maintain the claimed test level with a probability of 90 % an additional test level of 38 % percent must be added.
- b.) To maintain the claimed test level with a probability of 90 % an additional test level of 35 % percent must be added.
- c.) To maintain the claimed test level with a probability of 90 % an additional test level of 39 % percent must be added.
- d.) Measuring uncertainty (current): +/- 0,2% (fundamental oscillation), +/- 0,2% (rated current), voltage metering +/- 0,2% of the reading. Impacts on the measuring system by the EUT are not included.
- e.) Measuring uncertainty (flicker): dc and dmax +/- 5%, Pst +/- 8%. Impacts on the measuring system by the EUT are not included.



EMV **TESTHAUS** GmbH
Gustav-Hertz-Straße 35
94315 Straubing
Germany
Revision: 1.3

SOEKS Limited Liability Company
Nitrate testing device
NUC-019-1

130504-AU01+E02

Page 23 of 24

8. Summary

The EMC regulations according to the marked specifications are

☒ **Kept**

The Equipment under Test fulfills the general approval requirements mentioned.

☐ **Not kept**

The Equipment under Test does not fulfill the general approval requirements mentioned.

Straubing, January 21st, 2014



Martin Müller
Test engineer
EMV **TESTHAUS** GmbH



Christian Kiermeier
Technical executive
EMV **TESTHAUS** GmbH



EMV **TESTHAUS** GmbH
Gustav-Hertz-Straße 35
94315 Straubing
Germany
Revision: 1.3

SOEKS Limited Liability Company
Nitrate testing device
NUC-019-1

130504-AU01+E02

Page 24 of 24